

Verification of a novel point-of-care HbA_{1c} device in real world clinical practice by comparison to three high performance liquid chromatography instruments

Yufei Wang¹, Wei Peng², Junling Tang¹, Lu Dong¹, Chengchen Gu¹, Xin Zhang¹, Jian Zhou^{*3}, Weiping Jia^{1,3}

¹Shanghai Diabetes Institute, Shanghai Jiao Tong University Affiliated Sixth People's Hospital; Shanghai Key Laboratory of Diabetes Mellitus, Shanghai, China

²Wuxi Biohermes Bio&Medical Technology Co., Ltd., Wuxi, China

³Department of Endocrinology and Metabolism, Shanghai Jiao Tong University Affiliated Sixth People's Hospital, Shanghai Clinical Center for Diabetes, Shanghai Key Clinical Center for Metabolic Disease, Shanghai, China

The first two authors contributed equally to this work.

*Corresponding author: zhoujian@sjtu.edu.cn

Abstract

Introduction: A real world clinical study was designed and conducted to evaluate the performance of a novel point-of-care device for determination of glycated haemoglobin A_{1c} (HbA_{1c}), A1C EZ 2.0, in daily clinical practice.

Materials and methods: Five hundred and fourteen subjects were included in this study, and divided into three groups. HbA_{1c} was measured by A1C EZ 2.0 and three different high performance liquid chromatography (HPLC) devices: Bio-Rad Variant II Turbo, Tosoh HLC-723 G8 and Premier Hb9210 separately. Precision of A1C EZ 2.0 was also evaluated.

Results: Results obtained from A1C EZ 2.0 and all HPLC devices are correlated. Passing-Bablok regression analysis shows the equation of A1C EZ 2.0 results against the mean of HPLC devices with corresponding 95% confidence intervals (95% CI) for the intercept and slope is $y = 0.10 (-0.17 \text{ to } 0.10) + 1.00 (1.00 \text{ to } 1.04) x$. Bland-Altman difference plot shows that the mean relative difference between A1C EZ 2.0 and Variant II Turbo, G8, Hb9210 and all HPLC results is 2.5%, 0.6%, 0.4% and 1.1%, respectively. In addition, 121 pairs of results determined by using both venous and capillary blood prove that the difference of two kinds of blood sample causes no notable variation when measured by A1C EZ 2.0. Precision study gives 2.3% and 1.9% of total coefficient of variation for normal and abnormal HbA_{1c} sample in A1C EZ 2.0.

Conclusions: HbA_{1c} values measured by A1C EZ 2.0 were in good accordance with the results obtained with the reference HPLC devices.

Key words: point-of-care testing; glycated haemoglobin A1c; diabetes mellitus; evaluation studies

Received: August 25, 2017

Accepted: February 19, 2018

Introduction

Diabetes mellitus (DM) has become a cause of serious concern worldwide, as well as in China. The prevalence of DM and pre-diabetes among adult Chinese population in 2010 was estimated to be 11.6% and 50.1%, respectively, representing 113.9 and 493.4 million people. However, only 28.4% of DM patients have been diagnosed till now in China (1). This implies that over eighty million patients with undiagnosed DM still need to be screened and diagnosed, which can be a major challenge for the public health system of China. Glycated

haemoglobin A_{1c} (HbA_{1c}) values, which can reflect the average blood glucose concentration over the past 90-120 days, is now not only a standard index for evaluating the effectiveness of treatment, but also a widely acknowledged parameter for screening and diagnosing DM (2-4). High performance liquid chromatography (HPLC) is currently widely used for HbA_{1c} measurement in clinical practice, but it is generally used in the hospital central laboratory, where physician and patients have to wait for 1-3 days for getting the test results. Point-of-

care (POC) HbA_{1c} devices, which can provide test results within few minutes, is fast becoming a tool for the screening and diagnosis of DM at a relatively lower cost. Clinical studies have shown that POC devices help doctors in making timely adjustments in treatment plan, which further brings additional benefits to long-term glycaemic control (5-7). On the other hand, there were common concerns about the accuracy and precision of POC HbA_{1c} devices. Lenters-Westra *et al.* have studied the performance of eight POC HbA_{1c} devices in 2009, and only two of them met the generally accepted performance criteria (8). Most of POC HbA_{1c} devices in the study failed to achieve the total CV of 3%, and show notable differences of analytical performance between different reagent lots. A similar investigation of seven POC HbA_{1c} devices has been performed by the same authors in 2014 (9). Generally, significant improvement has been found in precision and accuracy of these devices, four of seven devices met the generally accepted performance criteria, though some specific problems, such as interferences or choice of reference device for calibration has been found in this study (9).

Here, we performed systematic evaluation of a novel hand-held HbA_{1c} POC device, A1C EZ 2.0 (Bi-ohermes, Wuxi, China; measurement range 4~14% HbA_{1c}) in a clinical study by comparison to HPLC instruments. Zhou *et al.* reported a study of A1C EZ 2.0 when our investigation was in progress, and their results show this device has favourable performances (10). In order to minimize the potential random bias caused by a definite reference device, three HPLC instruments were involved in our study, and their mean result for each sample, as well as test results by individual HPLC instruments, were used as reference values for comparison. Linear regression analysis, bias plot, as well as sensitivity and specificity analysis of A1C EZ 2.0 were performed based on the data obtained in the comparison study. In addition, the precision of A1C EZ 2.0 was also evaluated in this study. All instruments used in this study were certified by both the National Glycohemoglobin Standardization Program (NGSP) and the International Federation of Clinical Chemistry and Laboratory Medicine (IFCC) in 2016.

Materials and methods

Study design

We performed an analytical verification study of the POC HbA_{1c} device A1C EZ 2.0 by comparison with three other IFCC certified secondary reference method (SRM) HPLC instruments. Blood samples were collected from subjects in hospital, and the study lasted for seven months (detail information of instruments and subjects are given below).

Both venous and fingertip blood samples were used in the comparison, to investigate the test results difference between A1C EZ 2.0 and three HPLC instruments. Potential difference of test results caused by sample types was also studied by testing both venous and fingertip blood from the same subjects in the same instrument in this study.

We also evaluated the precision of A1C EZ 2.0 following CLSI EP5-A2 (Evaluation Of Precision Performance Of Quantitative Measurement Methods. Approved Guideline - Second Edition). Two potassium-ethylenediaminetetraacetic acid (K₂-EDTA) anticoagulant whole blood samples (one within normal range and the other in the higher range of HbA_{1c} values) were tested in two runs per day in duplicate on twenty consecutive days. Controls provided by manufacturers were used before and after every day's experiments to ensure that performance of all instruments meets the required standards by manufacturers. Otherwise calibration was carried out following manufacturers' manual.

Subjects

After approval from the institutional review committee of Shanghai Jiao Tong University Affiliated Sixth People's Hospital (Shanghai, China), and in accordance with the principles of the Helsinki Declaration II, we randomly recruited 514 subjects from the Outpatient Departments of the Endocrinology and Metabolism of Shanghai Jiao Tong University Affiliated Sixth People's Hospital. We included both diabetes and non-diabetes cases aged fourteen and older. We excluded specimens from subjects with anaemia, haemolytic disease, red cell cycle abnormalities, nephropathy and other known comorbidities.

ties, whose diseases were reported through a questionnaire survey or determined by relevant laboratory results. Subjects aged 60 (15 - 93) were enrolled from April to October 2016. Median age of male and female subjects was 61 and 60, respectively.

All subjects have signed informed consent before their blood sample being collected. Subjects were divided into three groups, venous blood samples were collected from 197 subjects (subject group I, SGI), fingertip capillary whole blood samples were collected from other 196 subjects (subject group II, SGII), and both venous blood samples and fingertip capillary whole blood samples were collected from the rest 121 subjects (subject group III, SGIII).

Sample collection

All venous blood samples were collected in the standard tube (3mL, WeiGao Group, China) containing K₂-EDTA anticoagulant, stored at 4 °C and then tested within 24 hours of collection. One tube of venous blood sample was collected from each subject in SG I and SG III. For subjects in SG II, the fingertip capillary whole blood samples were directly used for the tests by A1C EZ 2.0, fingertip capillary whole blood samples were also collected in one mini tube containing K₂-EDTA anticoagulant and tested with three the HPLC devices within 24 hours.

Methods

The HbA_{1c} values from each blood sample were measured by A1C EZ 2.0 and all three HPLC devices: Bio-Rad Variant II Turbo (Bio-Rad Laboratories, Hercules, USA; measurement range 3.5 - 19% HbA_{1c}), Tosoh HLC-723 G8 (Tosoh, Tokyo, Japan; measurement range 4 - 16.9% HbA_{1c}) and Premier Hb9210 (Trinity Biotech, Bray, Ireland; measurement range 3.7 - 18.5% HbA_{1c}). Both A1C EZ 2.0 and Premier Hb9210 utilize boronate affinity method; however, A1C EZ 2.0 uses lateral chromatography on a porous membrane matrix, while Premier Hb9210 HPLC device uses column chromatography. Tosoh HLC-723 G8 and Bio-Rad Variant II Turbo devices utilize cation-exchange method. All tests were performed according to the manufacturers' instructions manual. Operators performing tests on the A1C EZ 2.0 and

HPLC devices were blinded to the clinical characteristics of the subjects.

Statistical analysis

Linear regression analysis

Passing-Bablok linear regression analysis of HbA_{1c} values obtained by A1C EZ 2.0 versus three HPLCs was further conducted to assess the accuracy of A1C EZ 2.0 while considering the above mentioned HPLC devices as references (11). The linear regression analysis in each subject group was performed separately. Six hundred and thirty-five pairs of data from all 514 subjects (121 subjects tested both venous blood and fingertip capillary whole blood) were also combined for linear regression analysis for each reference HPLC device. Finally, to check overall agreement independent of chosen reference HPLC device, the mean HbA_{1c} values of three HPLC devices (referred as "mean SRM" below) were used to perform the linear regression against results given by A1C EZ 2.0.

Bias plot, absolute value of relative difference and mean absolute value of relative difference

Bland-Altman difference plot was performed to evaluate the difference between the HbA_{1c} values given by A1C EZ 2.0 and HPLC devices (12). Mean difference as well as the mean relative difference between A1C EZ 2.0 results and each HPLC results were calculated. The limits of agreement for the difference between A1C EZ 2.0 and each HPLC device were also calculated to reflect the distribution of these differences. In addition, the absolute value of relative difference (ARD) analysis and mean absolute value of relative difference (MARD) analysis was performed. Absolute value of relative difference and MARD were calculated by using the following equations:

$$\text{ARD} = (|\text{A1C EZ 2.0 value} - \text{HPLC value}| / \text{HPLC value}) \times 100\%$$

$$\text{MARD} = \text{Average (ARD)}.$$

The distribution of the difference was further analysed based on the data of ARD and MARD. Six hundred and thirty-five pairs of data from all 514 subjects were combined and used for bias plot, ARD and MARD analysis.

Precision

Precision of A1C EZ 2.0 was evaluated using CLSI EP5-A2. The calculation of within-run, between-run, within-day and total coefficient of variance was followed by the standard method provided in CLSI EP5-A2.

Comparison of venous blood results and fingertip capillary whole blood results

Values of 121 pairs of venous blood and fingertip capillary whole blood on A1C EZ 2.0 were compared by Passing-Bablok linear regression analysis, to see if there is a significant difference between the two kinds of blood samples.

Sensitivity and specificity analysis

Sensitivity and specificity were calculated by using HbA_{1c} clinical decision limit for DM diagnosis of 6.5% and mean SRM or Premier Hb9210 as reference value. MedCalc (Ostend, Belgium) statistical software (version 16.4) was used to perform statistical analyses.

Results

Overall results

A total of 514 subjects, including 266 men and 248 women, were randomly recruited in this study. The venous and fingertip capillary whole blood were tested in the SGI (N = 197) and SGII (N = 196) group, respectively. SGIII (N = 121) subjects had

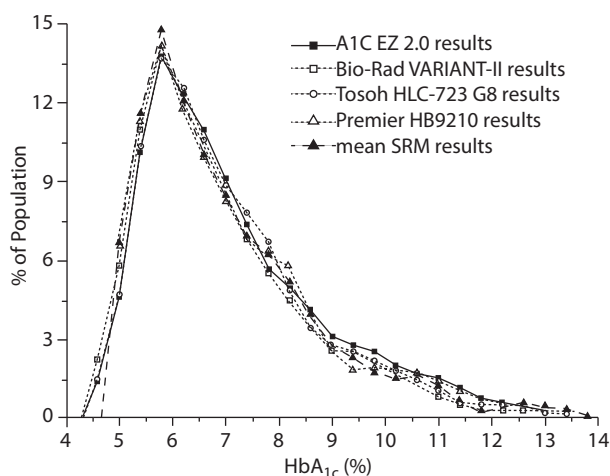


FIGURE 1. Frequency distribution of the HbA_{1c} values measured by the A1C EZ 2.0 and three secondary reference methods based on HPLC methodology including Bio-Rad Variant II Turbo, Tosoh HLC-723 G8 and Premier Hb9210. Distribution of mean SRM is also included in the figure. In total, 635 samples were analyzed by each instrument. The population percentage (y-axis) is plotted against HbA_{1c} values (x-axis).

evaluations of both venous blood and fingertip capillary whole blood.

The frequency distribution patterns of HbA_{1c} values for all four instruments were similar (Figure 1). HbA_{1c} values of all subjects ranged from 4.4 - 13.0% for A1C EZ 2.0 and from 4.5 - 13.6% for mean SRM, *i.e.* mean of all three HPLC devices. Median (95% confidence intervals, CIs) HbA_{1c} of A1C EZ 2.0 was 6.9% (6.7 - 7.0), and 6.7% (6.6 - 6.9) for all three HPLC devices put together (mean SRM) (Table 1).

TABLE 1. HbA_{1c} results for all the devices investigated

	A1C EZ 2.0	Bio-Rad VARIANT-II	Tosoh HLC-723 G8	Premier HB9210	Mean SRM
HbA1c range (%)	4.4 - 13.0	4.4 - 13.2	4.4 - 13.3	4.7 - 14.3	4.5 - 13.6
Median (95% CI)	6.9 (6.7 - 7.0)	6.7 (6.5 - 6.9)	6.8 (6.6 - 7.0)	6.8 (6.6 - 6.9)	6.7 (6.6 - 6.9)
KS test	P < 0.001	P < 0.001	P < 0.001	P < 0.001	P < 0.001
Skewness coefficients	1.062 (P < 0.001)	1.190 (P < 0.001)	1.199 (P < 0.001)	1.282 (P < 0.001)	1.226 (P < 0.001)
Kurtosis coefficients	0.678 (P = 0.011)	1.312 (P < 0.001)	1.348 (P < 0.001)	1.539 (P < 0.001)	1.388 (P < 0.001)

KS test - Kolmogorov-Smirnov test for normal distribution. Skewness coefficients and Kurtosis coefficients were used for normal distribution determination. SRM - secondary reference method.

TABLE 2. Regression analysis of A1C EZ 2.0 results versus three secondary reference methods and the mean SRM

Comparison of A1C EZ 2.0 vs. Bio-Rad VARIANT-II			
	Passing-Bablok regression equation, y = a (95% CI) + b (95% CI) x	Mean difference (limits of agreement)	Mean relative difference, % (limits of agreement)
All subjects	y = 0.03 (- 0.14 to 0.20) + 1.02 (1.00 to 1.05) x	0.17 (- 0.52 - 0.85)	2.5 (- 7.3 - 12.4)
SGI (venous group)	y = 0.30 (- 0.12 to 0.30) + 1.00 (1.00 to 1.06) x	0.24 (- 0.41 - 0.89)	3.4 (- 5.4 - 12.2)
SGII (capillary group)	y = - 0.36 (- 0.65 to 0.10) + 1.06 (1.00 to 1.10) x	0.06 (- 0.64 - 0.75)	0.7 (- 8.5 - 10.0)
SGIII (for venous)	y = - 0.10 (- 0.39 to 0.30) + 1.06 (1.00 to 1.10) x	0.24 (- 0.36 - 0.83)	3.8 (- 5.1 - 12.7)
SGIII (for capillary)	y = 0.20 (- 0.33 to 0.20) + 1.00 (1.00 to 1.09) x	0.16 (- 0.58 - 0.90)	2.7 (- 8.9 - 14.2)
Comparison of A1C EZ 2.0 vs. Tosoh HLC-723 G8			
All subjects	y = - 0.12 (- 0.27 to 0.00) + 1.02 (1.00 to 1.05) x	0.04 (- 0.57 - 0.66)	0.6 (- 8.0 - 9.2)
SGI (venous group)	y = 0.10 (0.04 to 0.10) + 1.00 (1.00 to 1.02) x	0.09 (- 0.51 - 0.69)	1.3 (- 6.6 - 9.3)
SGII (capillary group)	y = - 0.46 (- 0.76 to 0.00) + 1.06 (1.00 to 1.11) x	- 0.04 (- 0.72 - 0.65)	- 0.6 (- 9.6 - 8.4)
SGIII (for venous)	y = - 0.32 (0.59 to 0.10) + 1.06 (1.00 to 1.10) x	0.08 (- 0.44 - 0.60)	1.1 (- 6.8 - 9.0)
SGIII (for capillary)	y = - 0.20 (0.52 to 0.00) + 1.04 (1.00 to 1.09) x	0.05 (- 0.52 - 0.63)	0.8 (- 8.1 - 9.7)
Comparison of A1C EZ 2.0 vs. Tosoh HLC-723 G8 Premier HB9210			
All subjects	y = 0.00 (- 0.00 to 0.00) + 1.00 (1.00 to 1.00) x	0.02 (- 0.57 - 0.61)	0.4 (- 7.3 - 8.2)
SGI (venous group)	y = 0.22 (0.00 to 0.43) + 0.97 (0.94 to 1.00) x	- 0.05 (- 0.67 - 0.56)	- 0.4 (- 8.0 - 7.2)
SGII (capillary group)	y = 0.00 (- 0.25 to 0.00) + 1.00 (1.00 to 1.04)x	0.00 (- 0.64 - 0.65)	0.2 (- 7.8 - 8.2)
SGIII (for venous)	y = - 0.29 (- 0.54 to - 0.10) + 1.06 (1.00 to 1.10) x	0.11 (- 0.34 - 0.56)	1.6 (- 5.4 - 8.6)
SGIII (for capillary)	y = - 0.37 (- 0.64 to - 0.11) + 1.07 (1.02 to 1.11) x	0.07 (- 0.44 - 0.58)	1.0 (- 6.7 - 8.8)
Comparison of A1C EZ 2.0 vs. mean SRM			
All subjects	y = 0.10 (- 0.17 to 0.10) + 1.00 (1.00 to 1.04) x	0.08 (- 0.50 - 0.65)	1.1 (- 6.9 - 9.2)
SGI (venous group)	y = 0.10 (0.10 to 0.10) + 1.00 (1.00 to 1.00) x	0.09 (- 0.48 - 0.67)	1.4 (- 6.1 - 9.0)
SGII (capillary group)	y = - 0.30 (- 0.56 to 0.00) + 1.05 (1.00 to 1.08) x	0.01 (- 0.63 - 0.64)	0.1 (- 8.2 - 8.4)
SGIII (for venous)	y = - 0.22 (- 0.49 to 0.10)+ 1.06 (1.00 to 1.10) x	0.14 (- 0.33 - 0.61)	2.1 (- 5.1 - 9.4)
SGIII (for capillary)	y = - 0.23 (- 0.54 to 0.10) + 1.05 (1.00 to 1.10) x	0.09 (- 0.44 - 0.63)	1.4 (- 7.0 - 9.8)

Linear regression

Linear regression analysis indicates that test results of A1C EZ 2.0 show good agreement with the results obtained by reference HPLC devices (Table 2). The linear regression equation of A1C EZ 2.0 values against mean SRM is presented in Figure 2. A1C EZ 2.0 is most closely related to Premier Hb9210 of all the three reference HPLC devices. The slope and intercept given by linear regression between A1C EZ 2.0 and Premier Hb9210 with all of the combined data is 1.00 (1.00 to 1.00) and 0.00 (-0.00 to 0.00), respectively, which coincides with the ideal $y = x$ function.

Bias analysis

The mean difference between A1C EZ 2.0 values versus mean SRM is 0.08% HbA_{1c} (mean relative difference of 1.1%) (Figure 3 and Table 2). Respective mean difference for each reference HPLC device was 0.17% HbA_{1c} for Bio-Rad Variant II Turbo, 0.04% HbA_{1c} for Tosoh HLC-723 G8 and 0.02% HbA_{1c} for Premier Hb9210 (mean relative difference of 2.5%, 0.6% and 0.4%, respectively). All detailed statistics for each subject group are listed in Table 2. Bland-Altman difference plot of A1C EZ 2.0 results vs mean SRM shows that 96.5% of results have relative differences from -6.9% to 9.2% (Figure 3). In addition, 84.6% of data has ARD lower than 6%, and 94.2% of data has ARD lower than 8%. MARD of 3.26% of A1C EZ 2.0 results compared with mean SRM was found.

Differences in HbA_{1c} values depending upon types of blood sample

In this study, no notable difference in HbA_{1c} values between venous and fingertip capillary whole blood of SGIII subjects was seen as measured by A1C EZ 2.0. Passing-Bablok regression analysis towards paired data from venous and fingertip capillary whole blood yielded the equation $y = -0.10 + 1.00x$; with 95%CI of intercept -0.10 to 0.08, and slope: 0.98 to 1.00, which indicates that there is no significant difference between HbA_{1c} values on measurement with different kinds of blood sample. Also, there was no significant difference in

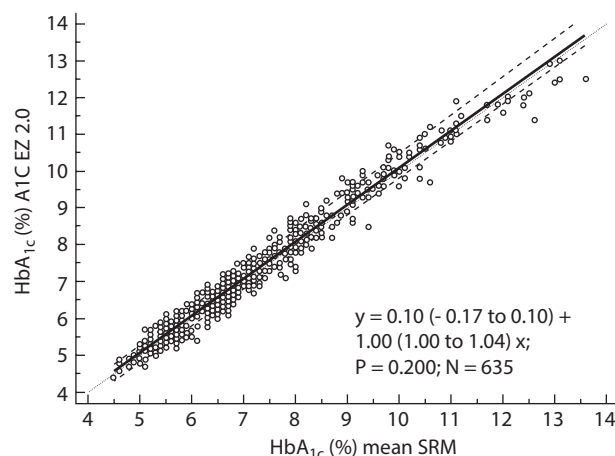


FIGURE 2. Scatter diagram and linear regression analysis of A1C EZ 2.0 results versus mean SRM. The regression line (solid line), 95% CIs (dashed lines) and the identity line ($y = x$, dotted line) are displayed. SRM- secondary reference method.

HbA_{1c} values between venous and capillary blood on assessment with reference HPLC devices (Bio-Rad Variant II Turbo: $y = 0.00 (0.00 \text{ to } 0.00) + 1.00 (1.00 \text{ to } 1.00) x$; Tosoh HLC-723 G8: $y = 0.0 (0.00 \text{ to } 0.00) + 1.0 (1.00 \text{ to } 1.00) x$; Premier Hb9210: $y = 0.0 (0.00 \text{ to } 0.00) + 1.00 (1.00 \text{ to } 1.00) x$).

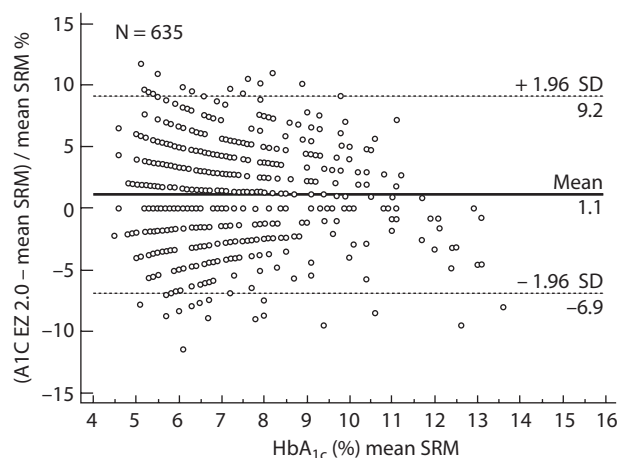


FIGURE 3. Bland-Altman relative difference plot shows the differences between the paired A1C EZ 2.0 results and the mean SRM. Horizontal lines are drawn at the mean difference% (solid line) and at the limits of agreement (dashed lines). Mean relative difference of A1C EZ 2.0 results versus the mean SRM is 1.1%, with the limits of agreement from -6.9% to 9.2%. SRM- secondary reference method.

TABLE 3. Coefficients of variation calculated according to CLSI EP5-A2

CV (%)	Sample 1 (HbA _{1c} = 5.2%)	Sample 2 (HbA _{1c} = 11.6%)
Within-run	1.9%	1.8%
Between-run	0.0%	0.6%
Between-day	1.4%	0.0%
Total	2.3%	1.9%

CV – coefficient of variation.

Precision

A1C EZ 2.0 showed good precision in the twenty days evaluation period (Table 3). The total CV is 2.3% for low HbA_{1c} sample (5.2% HbA_{1c}) and 1.9% for high HbA_{1c} sample (11.6% HbA_{1c}). In addition, the within-run CV, between-run CV and between-day CV all fell in the acceptable region (less than 2%, Table 3), implying that A1C EZ 2.0 has consistent performance over a certain period of time under different circumstances.

Sensitivity and specificity of test by A1C EZ 2.0

We further evaluated the sensitivity and specificity of A1C EZ 2.0. While considering Premier Hb9210 results as reference and HbA_{1c} of 6.5% as clinical decision level for DM diagnosis, the sensitivity and specificity of A1C EZ 2.0 were both 96%. When mean SRM was used as reference, sensitivity and specificity of A1C EZ 2.0 were 96% and 93%, respectively (Table 4).

Discussion

A large scale clinical study in the hospital setting was designed to evaluate the performance of a novel POC HbA_{1c} device A1C EZ 2.0. Overall performance of A1C EZ 2.0 was fairly good in our study, and was similar to the previously reported performance by another study (7). What is different is that in this study we used the clinical specimens including the fingertip capillary whole blood, venous blood samples and both venous blood samples and fingertip capillary whole blood samples from the same participant. Analysis of our results indicates that A1C EZ 2.0 has smallest mean difference (0.02% HbA_{1c}) with Premier Hb9210, and slightly less consistence with Tosoh HLC-723 G8 and Bio-Rad Variant II Turbo. This might be as both A1C EZ 2.0 and Premier Hb9210 use boronate affinity method. Boronate affinity method was proven to have good tolerance to some common interference factors such as haemoglobin variants and certain drugs, which usually affect the HbA_{1c} results determined by cation-exchange method (13,14). In this study, sample from one patient (data was excluded in our statistics) was found to have haemoglobin abnormality and both Bio-Rad Variant II Turbo and Tosoh HLC-723 G8 failed to give reasonable results, while Premier Hb9210 and A1C EZ 2.0 gave similar HbA_{1c} value (7.6% and 7.8% HbA_{1c}, respectively). For several other samples where the relative differences between Premier Hb9210 and Tosoh HLC-723 G8 or Bio-Rad Variant II Turbo were more than 10%, we inferred that some interference factors might have existed in those samples and Premier Hb9210 results were considered to be more reliable.

TABLE 4. Diagnostic sensitivity and specificity of A1C EZ 2.0 for diagnosing of diabetes

HbA _{1c} cut-off value		A1C EZ 2.0 vs. Bio-Rad VARIANT-II	A1C EZ 2.0 vs. Tosoh HLC-723 G8	A1C EZ 2.0 vs. Premier HB9210	A1C EZ 2.0 vs. mean SRM
6.5%	Sensitivity (%)	96	95	96	96
	Specificity (%)	90	96	96	93
6.3%	Sensitivity (%)	97	95	96	97
	Specificity (%)	87	92	89	89

SRM- secondary reference method.

Although venous blood may differ from capillary blood to some extent, in many aspects, such as total protein, blood cell concentration and ion concentration, the HbA_{1c} value usually shows no notable difference when measured using different type of blood sample in different instruments (15-19). There was no significant difference in HbA_{1c} values between venous blood and fingertip capillary whole blood of SGIII subjects as seen on measurement by A1C EZ 2.0.

Sensitivity and specificity analysis of A1C EZ 2.0 indicates that the risk of false positive and negative results is very low with evaluation by A1C EZ 2.0. Several former studies have shown that the ideal cut-off HbA_{1c} values for diagnosis of DM varies among ethnic groups, and the best clinical decision level for Chinese population might be 6.3% (20-23). We also used 6.3% as cut-off value, and found that the sensitivity and specificity of A1C EZ 2.0 was 96% and 89% as compared to Premier Hb9210 as reference, and 97% and 89% as compared to mean SRM as reference. In this analysis, when clinical decision level was changed from 6.5% to 6.3%, high sensitivity was maintained, whereas specificity dropped as compared to both references (Table 4). In conclusion, the sensitivity and specificity of A1C EZ 2.0 meets the general clinical requirement for HbA_{1c} testing, and can be used for clinical diabetes diagnosis.

As the POC HbA_{1c} devices can provide results in short time and at relatively lower cost, these can help in improving the doctor-patient interaction, appropriate modification of the treatment if required and/or diagnosis/screening of new cases of DM from large population with higher efficiency. On the other hand, doubts towards POC HbA_{1c} devices have been raised in some studies showing that some POC HbA_{1c} devices may not be suitable for clinical use due to their unsatisfactory precision and/or variation in different lots (5,6). Thus, more precise and accurate POC HbA_{1c} device is in urgent need, especially in countries like China, with an increasing incidence and prevalence of DM, as expensive HPLC HbA_{1c} instruments are usually inaccessible and unaffordable to many grassroots medical institutions.

While it is widely accepted that HPLC devices represent one of the most accurate way to measure HbA_{1c}, we found that performance of POC HbA_{1c} device is not significantly different from the HPLC devices in this study. The 84.7% of Bio-Rad Variant II Turbo results have ARD lower than 6%, and 94.6% have lower than 8% as compared with Premier Hb9210 results. Both values are slightly lower than A1C EZ 2.0 87.6% and 96.5%, respectively (data not shown). The controls were tested before and after every day's experiments and routine calibrations were carried out in all HPLC devices to confirm that performance of all instruments were in the claimed acceptable region by manufacturers. However, Bio-Rad Variant II Turbo results show consistent negative bias (about - 0.2% HbA_{1c}) as compared with Tosoh HLC-723 G8, Premier Hb9210, A1C EZ 2.0 in our study. This negative bias was observed in all three subject groups and through seven months period of this study. Such kind of bias might have occurred due to the change of condition of cation-exchange column during use, or the individual calibration process we performed, as both are commonly seen in clinical applications. On the other hand, use of POC HbA_{1c} device like A1C EZ 2.0, which usually uses single cartridge or strip for one test can decrease the risk of systematic bias and might achieve similar performance as HPLC in clinical practice while having slightly higher CV than HPLC device at the same time.

In conclusion, we verified a novel POC HbA_{1c} device A1C EZ 2.0, and found its performance met the general clinical requirement in this study. However, there are still some limitations in our study. Only one lot of strip of A1C EZ 2.0 was used in this study, thus lot-to-lot variation of strips has not been evaluated; we also did not evaluate the stability of test strip of A1C EZ 2.0 in this work. Tests by A1C EZ 2.0 and HPLC instruments were not performed at exactly the same point of time. All these limitations merit further investigation in future.

Acknowledgments

We are very grateful to all the staff for helping with the present study. We are grateful to all participants for their dedication in data collection and

laboratory measurements. This work was funded by the Shanghai Municipal Education Commission—Gaofeng Clinical Medicine Grant Support (20161430), and the innovation foundation of translational medicine of Shanghai Jiao Tong Uni-

versity School of Medicine and Shanghai SJTUSM Biobank (15ZH4006).

Potential conflict of interest

None declared.

References

- Xu Y, Wang L, He J, Bi Y, Li M, Wang T, et al. Prevalence and control of diabetes in Chinese adults. *JAMA* 2013;310:948–59. <https://doi.org/10.1001/jama.2013.168118>
- Weykamp C, John WG, Mosca A. A review of the challenge in measuring hemoglobin A1c. *J Diabetes Sci Technol* 2009;3:439–45. <https://doi.org/10.1177/193229680900300306>
- Nathan DM, Singer DE, Hurxthal K, Goodson JD. The clinical information value of the glycosylated hemoglobin assay. *N Engl J Med* 1984;310:341–6. <https://doi.org/10.1056/NEJM198402093100602>
- Dreval AV, Cheporeva ON, Red'kin luA, Misnikova IV. Correlation of HbA(1c) and postprandial glycemia during a standard breakfast test in patients with type 2 diabetes mellitus receiving glibenclamide. *Ter Arkh* 2010;82:41–4. (in Russian)
- Cagliero E, Levina EV, Nathan DM. Immediate feedback of HbA1c levels improves glycemic control in type 1 and insulin-treated type 2 diabetic patients. *Diabetes Care* 1999;22:1785–9. <https://doi.org/10.2337/diacare.22.11.1785>
- Ferenczi A, Reddy K, Lorber DL. Effect of immediate hemoglobin A1c results on treatment decisions in office practice. *Endocr Pract* 2001;7:85–8. <https://doi.org/10.4158/EP.7.2.85>
- Miller CD, Barnes CS, Phillips LS, Ziemer DC, Gallina DL, Cook CB, et al. Rapid A1c availability improves clinical decision-making in an urban primary care clinic. *Diabetes Care* 2003;26:1158–63. <https://doi.org/10.2337/diacare.26.4.1158>
- Lenters-Westra E, Slingerland RJ. Six of eight hemoglobin A1c point-of-care instruments do not meet the general accepted analytical performance criteria. *Clin Chem* 2009;56:44–52. <https://doi.org/10.1373/clinchem.2009.130641>
- Lenters-Westra E, Slingerland RJ. Three of 7 hemoglobin A1c point-of-care instruments do not meet generally accepted analytical performance criteria. *Clin Chem* 2014;60:1062–72. <https://doi.org/10.1373/clinchem.2014.224311>
- Zhou R, Wang W, Song ZX, Tong Q, Wang QT. Evaluation of a new hemoglobin A1c analyzer for point-of-care testing. *J Clin Lab Anal* 2018;32:e22172. <https://doi.org/10.1002/jcla.22172>
- Bilić-Zulle L. Comparison of methods: Passing and Bablok regression. *Biochem Med (Zagreb)* 2011;21:49–52. <https://doi.org/10.11613/BM.2011.010>
- Altman DG, Bland JM. Measurement in medicine: the analysis of method comparison studies. *The Statistician* 1983;32:307–17. <https://doi.org/10.2307/2987937>
- Bry L, Chen PC, Sacks DB. Effects of hemoglobin variants and chemically modified derivatives on assays for glycohemoglobin. *Clin Chem* 2001;47:153–63.
- Lin CN, Emery TJ, Little RR, Hanson SE, Rohlfing CL, Jai-sson S, et al. Effects of hemoglobin C, D, E, and S traits on measurements of HbA1c by six methods. *Clin Chim Acta* 2012;413:819–21. <https://doi.org/10.1016/j.cca.2011.12.019>
- Kupke IR, Kather B, Zeugner S. On the composition of capillary and venous blood serum. *Clin Chim Acta* 1981;112:177–85. [https://doi.org/10.1016/0009-8981\(81\)90376-4](https://doi.org/10.1016/0009-8981(81)90376-4)
- Font MT, Brichs MC, Alvarez MC, Olivella JM, Turo JS, Fernandez MP. Capillary HbA1c determination on type 2 diabetes patients in a primary health centre. *Aten Primaria* 2011;43:536–43.
- Valdivia Perez A, Rico Blazquez M, Luis Martin F, Mingo Plaza D, Lozano Garcia I, Pizarro Blanco M. Assessment of HbA1c in capillary blood compared to venous blood. *Aten Primaria* 2010;42:126–7;author reply 128.
- Heylen O, Van Neyghem S, Exterbille S, Wehlou C, Gorus F, Weets I. Evaluation of the Sebia CAPILLARYS 2 flex piercing for the measurement of HbA(1c) on venous and capillary blood samples. *Am J Clin Pathol* 2014;141:867–77. <https://doi.org/10.1309/AJCPRU5QC2JBANSV>
- Keramati T, Razi F, Tootee A, Larijani B. Comparability of hemoglobin A1c level measured in capillary versus venous blood sample applying two point-of-care instruments. *J Diabetes Metab Disord* 2014;13:94. <https://doi.org/10.1186/s40200-014-0094-1>
- Eldeirawi K, Lipton RB. Predictors of hemoglobin A1c in a national sample of nondiabetic children: the Third National Health and Nutrition Examination Survey, 1988-1994. *Am J Epidemiol* 2003;157:624–32. <https://doi.org/10.1093/aje/kwg023>
- Olson DE, Rhee MK, Herrick K, Ziemer DC, Twombly JG, Phillips LS. Screening for diabetes and pre-diabetes with proposed A1C-based diagnostic criteria. *Diabetes Care* 2010;33:2184–9. <https://doi.org/10.2337/dc10-0433>
- Bao Y, Ma X, Li H, Zhou M, Hu C, Wu H, et al. Glycated haemoglobin A1c for diagnosing diabetes in Chinese population: cross sectional epidemiological survey. *BMJ* 2010;340:c2249. <https://doi.org/10.1136/bmj.c2249>
- Xin Z, Yuan MX, Li HX, Hua L, Feng JP, Shi J, et al. Evaluation for fasting and 2-hour glucose and HbA1c for diagnosing diabetes based on prevalence of retinopathy in a Chinese population. *PLoS One* 2012;7:e4061. <https://doi.org/10.1371/journal.pone.0040610>